Test Components

COVID-19 Ag

This is not a complete Instruction for use. For more detailed instructions, please refer to IFU.

COVID-19 Ag_Rev01_200706E



Test cartridge




Detector tube (Granule)



Extraction tube





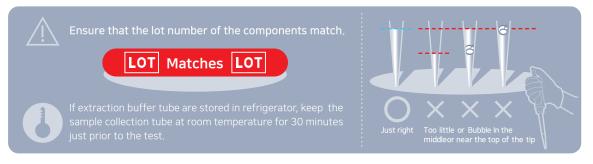

Test Setup

1 Turn the power switch 'On'



Insert ID chip



3 Press 'Multi-test'



Test Procedure


To collect the sample, insert a sterile swab in the nasal cavity and spin it smoothly in the nasopharynx.



Open the lid of the aluminum Insert the sterile swab used to foil of the extraction tube collect the sample into the extraction tube and swirl 5 times



While squeezing the tube, pull the swab out



Assemble the nozzle and the extraction tube



7 Shake 20 times












10 Insert the test cartridge



11 Press 'Start'



12 Read the test result





Pipette out 75 µL and load it into

the sample well on the cartridge



9 Wait 12 minutes

